EN

INSTRUCTIONS FOR USE

UDO HEISIG GMBH
THE DISPOSABLES COMPANY

UNIFLEX® TUR-Apron

NON STERILE

Intended purpose: OP device cover for collecting and draining liquids, for the duration of one application.
For mounting on the operating table. With neckline and table support.

1

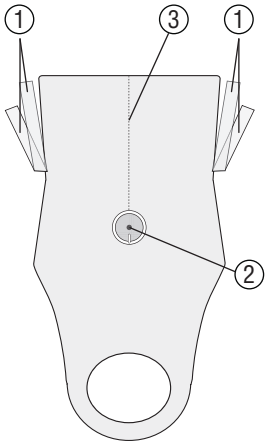

The TUR-Apron is unfolded in such a way that the fastening straps (1) are accessible. The discharge nozzle (2) points downwards (see also illustration 5), and the weld seam (3) points towards the operating table.

2

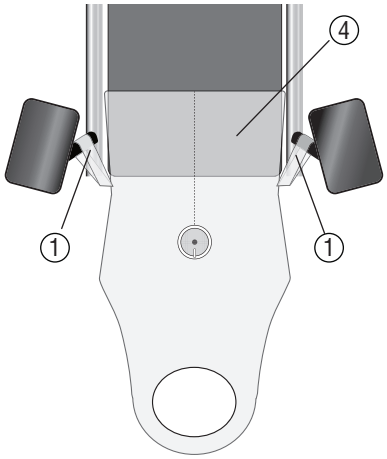

The fastening straps (1) are fixed to the operating table at a suitable location, and the area (4) for resting on the table is placed on the table.

3

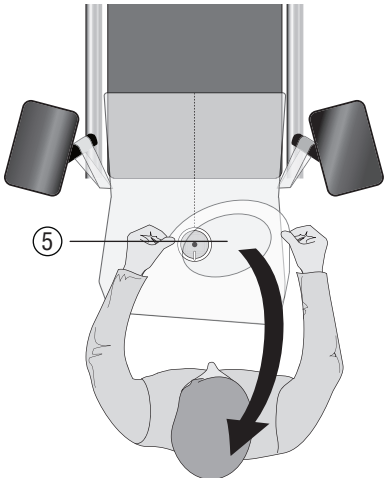

The neckline (5) of the Apron is pulled over the head of the user. If fastened correctly, the TUR-Apron cannot become detached by itself.

4

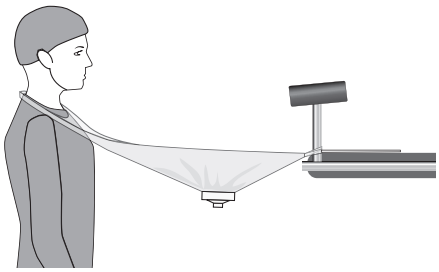

The neckline of the Apron, as worn.

5

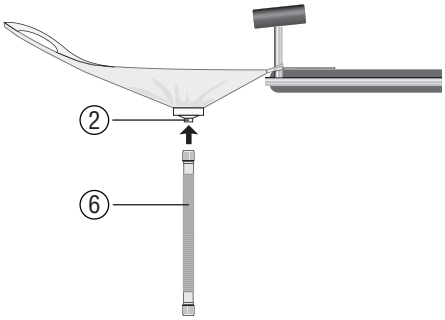

The (separately available) corrugated tube (6) can now be pushed onto the discharge nozzle (2) of the Apron.

6

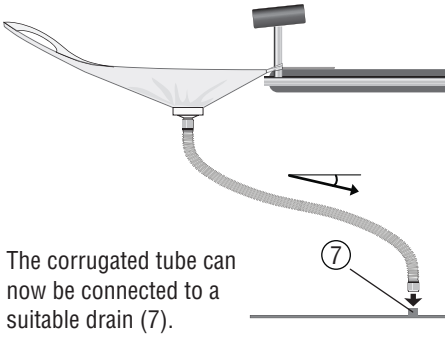

The corrugated tube can now be connected to a suitable drain (7).
To avoid liquid build-up, ensure a constant slope inside the drain hose.

Suitable adapters for the drain are available separately.

7

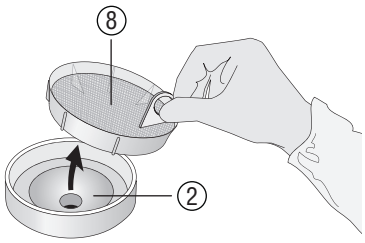

The filter sieve (7) holds back tissue fragments and thus prevents the conduit from becoming blocked. It can be removed from the discharge nozzle (2).

Date: 2022-09-15

Version: **P0138U EN Rev00**

UDO HEISIG GMBH
THE DISPOSABLES COMPANY
Hermann-Oberth-Str. 17
85640 Putzbrunn
Bavaria / Germany
Company management:
Udo Heisig, Carmen Silies
AG München, HRB 82813
Tel. +49 89 / 46 23 92 - 0
Fax +49 89 / 46 23 92 - 28
info@heisig.de | www.heisig.de

CE

PLEASE OBSERVE WARNINGS ON THE BACK

PACKAGE CONTENT		DETAILS
REF 37932U	UNIFLEX® TUR-Apron	Size: 70 x 125 cm
A detailed product specification is available on request.		

Corrugated tube **REF 32017U** (Inside diameter of adapter: 22 mm, length extendable up to 200 cm) is available separately.

WARNINGS and IMPORTANT INFORMATION

Do not use if the packaging is damaged

CAUTION: Do not use damaged products!

Do not reuse

CAUTION: Not suitable for reuse, as the required features may fail and cause an infection of the patient.

CAUTION: The instructions for use apply only **to the enclosed products.**

Store in a dry place

Keep away from direct sunlight

ATTENTION: To avoid liquid build-up inside the drain hose, ensure a **constant slope** inside the hose during installation.

CAUTION: To be used **only by healthcare professionals!**

CAUTION: Any **serious incident** that has occurred in relation to the device has to be reported to the manufacturer and the competent authority of the Member State in which the user and/or patient is established.

OTHER SYMBOLS USED

Non-sterile product

Use-by date

Latex-free

Consult instructions for use. The latest instructions for use can be downloaded at **www.heisig.de**

Personnel number of the manufacturing employee

Batch code
JJMM0123

Manufacturer

Number of products in a carton

Date of manufacture

Article number

PZN: 0000000 Pharmacy central number

Environmentally compatible if properly disposed of.
No toxic gases arise from burning.
Dump without groundwater pollution.

The product is compliant with valid legal requirements for medical devices

Medical device

UDO HEISIG GMBH
THE DISPOSABLES COMPANY
Hermann-Oberth-Str. 17
85640 Putzbrunn
Bavaria / Deutschland
Company management:
Udo Heisig, Carmen Silies
AG München, HRB 82813
Tel. +49 89 / 46 23 92 - 0
Fax +49 89 / 46 23 92 - 28
info@heisig.de | www.heisig.de